

**ITALY CONTACT:****Meridian Healthcare srl**

Via G. Guglielmino, 68 - 95030 Tremestieri Etneo - CT

Tel. 095 725 68 69 - Fax: 095 725 44 54

e-mail: info@meridianhealthcare.it

 Meridian Healthcare<sup>®</sup>**Instructions for use**  
**GABA ELISA**

Please use only the valid version of the Instructions for Use provided with the kit

**REF****BA E-2500****RUO**For research  
use only –  
Not for use  
in diagnostic  
procedures

## **1. Introduction**

### **1.1 Intended use and principle of the test**

Enzyme Immunoassay for the quantitative determination of Gamma-aminobutyric acid (GABA) in human plasma, serum, urine and various biological samples.

After extraction and derivatization Gamma-aminobutyric acid (GABA) is quantitatively determined by ELISA. The competitive ELISA uses the microtiter plate format. The antigen is bound to the solid phase of the microtiter plate. The derivatized analyte concentrations of the standards, controls and samples and the solid phase bound analyte compete for a fixed number of antiserum binding sites. When the system is in equilibrium, free antigen and free antigen-antibody complexes are removed by washing. The antibody bound to the solid phase is detected by an anti-rabbit IgG-peroxidase conjugate using TMB as a substrate. The reaction is monitored at 450 nm.

Quantification of unknown samples is achieved by comparing their absorbance with a standard curve prepared with known standards.

## **2. Procedural cautions, guidelines, warnings and limitations**

### **2.1 Procedural cautions, guidelines and warnings**

- (1) This kit is intended for professional use only. Users should have a thorough understanding of this protocol for the successful use of this kit. Only the test instruction provided with the kit is valid and has to be used to run the assay. Reliable performance will only be attained by strict and careful adherence to the instructions provided.
- (2) This assay was validated for a certain type of sample as indicated in *Intended Use* (please refer to Chapter 1). Any off-label use of this kit is in the responsibility of the user and the manufacturer cannot be held liable.
- (3) The principles of Good Laboratory Practice (GLP) have to be followed.
- (4) In order to reduce exposure to potentially harmful substances, wear lab coats, disposable protective gloves and protective glasses where necessary.
- (5) All kit reagents and specimens should be brought to room temperature and mixed gently but thoroughly before use. Avoid repeated freezing and thawing of reagents and specimens.
- (6) For dilution or reconstitution purposes, use deionized, distilled, or ultra-pure water.
- (7) The microplate contains snap-off strips. Unused wells must be stored at 2 °C to 8 °C in the sealed foil pouch with desiccant and used in the frame provided.
- (8) Duplicate determination of sample is highly recommended to be able to identify potential pipetting errors.
- (9) Once the test has been started, all steps should be completed without interruption. Make sure that the required reagents, materials and devices are prepared ready at the appropriate time.
- (10) Incubation times do influence the results. All wells should be handled in the same order and time intervals.
- (11) To avoid cross-contamination of reagents, use new disposable pipette tips for dispensing each reagent, sample, standard and control.
- (12) A standard curve must be established for each run.
- (13) The controls should be included in each run and fall within established confidence limits. The confidence limits are listed in the QC-Report provided with the kit.
- (14) Do not mix kit components with different lot numbers within a test and do not use reagents beyond expiry date as shown on the kit labels.
- (15) Avoid contact with Stop Solution containing 0.25 M H<sub>2</sub>SO<sub>4</sub>. It may cause skin irritation and burns. In case of contact with eyes or skin, rinse off immediately with water.
- (16) TMB substrate has an irritant effect on skin and mucosa. In case of possible contact, wash eyes with an abundant volume of water and skin with soap and abundant water. Wash contaminated objects before reusing them.
- (17) For information on hazardous substances included in the kit please refer to Safety Data Sheet (SDS). The Safety Data Sheet for this product is made available directly on the website of the manufacturer or upon request.
- (18) Kit reagents must be regarded as hazardous waste and disposed of according to national regulations.

### **2.2 Limitations**

Any inappropriate handling of samples or modification of this test might influence the results.

### 2.2.1 Interfering substances

#### Serum/Plasma

Samples containing precipitates or fibrin strands or which are haemolytic or lipemic might cause inaccurate results.

#### 24-hour urine

Please note the sample preparation! If the percentage of the final concentration of acid is too high, this will lead to incorrect results for the urine samples.

### 2.2.2 Drug interferences

There are no known substances (drugs) which ingestion interferes with the measurement of GABA level in the sample.

### 2.2.3 High-Dose-Hook effect

No hook effect was observed in this test.

## 3. Storage and stability

Store the unopened reagents at 2 - 8 °C until expiration date. Do not use components beyond the expiry date indicated on the kit labels. Once opened the reagents are stable for 1 month when stored at 2 - 8 °C. Once the resealable pouch has been opened, care should be taken to close it tightly with desiccant again.

## 4. Materials

### 4.1 Contents of the kit

<b>BA D-0090</b>	<b>FOILS</b>	<b>Adhesive Foil</b> - Ready to use
Contents:	Adhesive Foils in a resealable pouch	
Volume:	3 x 4 foils	
<b>BA D-0033</b>	<b>48</b>	<b>Macrotiter Plate</b> - Ready to use
Contents:	2 x 48 well plate, empty in a resealable pouch	
<b>BA E-2442</b>	<b>EXTRACT-PLATE 48</b>	<b>Extraction Plate</b> - Ready to use
Contents:	2 x 48 well plate, precoated with cation exchanger in a resealable pouch	
<b>BA E-0030</b>	<b>WASH-CONC 50x</b>	<b>Wash Buffer Concentrate</b> - Concentrated 50x
Contents:	Buffer with a non-ionic detergent and physiological pH	
Volume:	1 x 20 ml/vial, light purple cap	
<b>BA E-0040</b>	<b>CONJUGATE</b>	<b>Enzyme Conjugate</b> - Ready to use
Contents:	Goat anti-rabbit immunoglobulins conjugated with peroxidase	
Volume:	1 x 12 ml/vial, red cap	
<b>BA E-0055</b>	<b>SUBSTRATE</b>	<b>Substrate</b> - Ready to use
Contents:	Chromogenic substrate containing tetramethylbenzidine, substrate buffer and hydrogen peroxide	
Volume:	1 x 12 ml/black vial, black cap	
<b>BA E-0080</b>	<b>STOP-SOLN</b>	<b>Stop Solution</b> - Ready to use
Contents:	0.25 M sulfuric acid	
Volume:	1 x 12 ml/vial, light grey cap	
Hazards identification:		H290 May be corrosive to metals. H314 Causes severe skin burns and eye damage.
<b>BA E-2531</b>	<b>GABA</b>	<b>GABA Microtiter Strips</b> - Ready to use
Contents:	1 x 96 well (12x8) antigen precoated microwell plate in a resealable foil pouch with desiccant	

**BA E-2510** **AS GABA** **GABA Antiserum** - Ready to use

Contents: Rabbit anti- GABA antibody, blue coloured

Volume: 1 x 6 ml/vial, blue cap

**Standards and Controls** - Ready to use

Cat. no.	Component	Colour/Cap	Concentration ng/ml	Concentration nmol/l	Volume/Vial
<b>BA E-2501</b>	<b>STANDARD A</b>	white	0	0	4 ml
<b>BA E-2502</b>	<b>STANDARD B</b>	light yellow	75	727	4 ml
<b>BA E-2503</b>	<b>STANDARD C</b>	orange	250	2 425	4 ml
<b>BA E-2504</b>	<b>STANDARD D</b>	dark blue	750	7 275	4 ml
<b>BA E-2505</b>	<b>STANDARD E</b>	light grey	2 500	24 250	4 ml
<b>BA E-2506</b>	<b>STANDARD F</b>	black	7 500	72 750	4 ml
<b>BA E-2551</b>	<b>CONTROL 1</b>	light green	Refer to QC-Report for expected value and acceptable range!		4 ml
<b>BA E-2552</b>	<b>CONTROL 2</b>	dark red			4 ml

Conversion: GABA (ng/ml) x 9.7 = GABA (nmol/l)

Contents: Acidic buffer with non-mercury preservative, spiked with defined quantity of GABA

**BA E-2513** **ASSAY-BUFF** **Assay Buffer** - Ready to use

Contents: Buffer with non-mercury preservative

Volume: 1 x 20 ml/vial, yellow cap

**BA E-2428** **EQUA-REAG** **Equalizing Reagent** - Lyophilized

Contents: Lyophilized protein

Volume: 1 vial, brown cap

**BA E-2446** **D-REAGENT** **D-Reagent** - Ready to use

Contents: Crosslinking agent in dimethylsulfoxide

Volume: 1 x 4 ml/vial, white cap

**BA E-2458** **Q-BUFFER** **Q-Buffer** - Ready to use

Contents: TRIS buffer

Volume: 1 x 20 ml/vial, white cap

**BA E-2561** **I-BUFFER** **I-Buffer** - concentrated

Contents: Buffer with non-ionic detergent and non-mercury preservative

Volume: 1 x 4 ml/vial, light red cap

**BA E-2541** **ELUTION-BUFF** **Elution-Buffer** - Ready to use

Contents: Buffer with citric acid

Volume: 1 x 50 ml/vial, dark green cap

**BA E-2560** **DILUENT** **Diluent** - Ready to use

Contents: Buffer with acidic pH

Volume: 2 x 20 ml/vial, blue cap

**BA E-2787** **NAOH** **NaOH** - Ready to use

Contents: Sodium hydroxide solution

Volume: 1 x 2 ml/vial, purple cap

Hazards identification:



H290 May be corrosive to metals.  
H315 Causes skin irritation.  
H319 Causes serious eye irritation.

\*For the determination of serum and plasma, standards and controls should always be diluted 1:3 [e.g. 100 µl standard + 200 µl water (deionized, distilled, or ultra-pure)]. Do not forget to correct the result afterwards for the dilution. Urine values of GABA are higher than for serum and plasma. Dilution of the standards is to make sure sample is measured in linear part of standard curve.

#### 4.2 Additional materials and equipment required but not provided in the kit

- Calibrated precision pipettes to dispense volumes between 10 – 400 µl; 1 ml; 10 ml
- Microtiter plate washing device (manual, semi-automated or automated)
- ELISA reader capable of reading absorbance at 450 nm and if possible 620 - 650 nm
- Microtiter plate shaker (shaking amplitude 3 mm; approx. 600 rpm)
- Vortex mixer
- Absorbent material (paper towel)
- Water (deionized, distilled, or ultra-pure)

#### 5. Sample collection and storage

##### Plasma

Whole blood should be collected into centrifuge tubes containing EDTA as anti-coagulant (Monovette™ or Vacuette™ for plasma) and centrifuged according to manufacturer's instructions at room temperature immediately after collection.

Fasting specimens or pre-feed specimens for children (2 - 3 hours after last meal) are advised.

Haemolytic and especially lipemic samples should not be used for the assay.

Storage: up to 24 hours at 2 - 8 °C, for longer period (up to 6 month) at -20 °C.

Repeated freezing and thawing should be avoided.

##### Serum

Collect blood by venipuncture (Monovette™ or Vacuette™ for serum), allow to clot, and separate serum by centrifugation according to manufacturer's instructions at room temperature. Do not centrifuge before complete clotting has occurred. Patients receiving anticoagulant therapy may require increased clotting time.

Fasting specimens or pre-feed specimens for children (2 - 3 hours after last meal) are advised.

Haemolytic and especially lipemic samples should not be used for the assay.

Storage: up to 24 hours at 2 - 8 °C, for longer period (up to 6 month) at -20 °C.

Repeated freezing and thawing should be avoided.

##### Urine

Spontaneous urine or 24-hour urine, collected in a bottle containing 10 - 15 ml of 6 M HCl, can be used.

If 24-hour urine is used please record the total volume of the collected urine.

Storage: for longer periods (up to 6 month) at -20 °C.

Repeated freezing and thawing should be avoided. Avoid exposure to direct sunlight!

#### 6. Test procedure

Allow all reagents and samples to reach room temperature and mix thoroughly by gentle inversion before use. Duplicate determinations are recommended. It is recommended to number the strips of the microwell plate before usage to avoid any mix-up.

The binding of the antisera and of the enzyme conjugate and the activity of the enzyme are temperature dependent, and the absorption values may vary if a thermostat is not used. The higher the temperature, the higher the absorption values will be. Varying incubation times will have similar influences on the absorbance. The optimal temperature during the Enzyme Immunoassay is between 20 – 25 °C.

⚠ In case of overflow, read the absorbance of the solution in the wells within 10 minutes, using a microplate reader set to 405 nm

#### 6.1 Preparation of reagents

##### Wash Buffer

Dilute the 20 ml Wash Buffer Concentrate with water (deionized, distilled, or ultra-pure) to a final volume of 1000 ml.

Storage: 1 month at 2 – 8 °C

##### Equalizing Reagent

Reconstitute the Equalizing Reagent with **10 ml** of **Assay Buffer**.

Reconstituted Equalizing Reagent which is not used immediately has to be stored in aliquots for max 1 month at -20 °C and may be thawed only once.

##### I-Buffer

Dilute the 4 ml I-Buffer Concentrate with water (deionized, distilled, or ultra-pure) to a final volume of 400 ml.

Storage: 1 month at 2 – 8 °C

### D-Reagent

The D-Reagent has a freezing point of 18.5 °C. Make sure that the D-Reagent has reached room temperature and forms a homogeneous, crystal-free solution.

### GABA Microtiter Strips

In rare cases residues of the blocking and stabilizing reagent can be seen in the wells as small, white dots or lines. These residues do not influence the quality of the product.

## 6.2 Preparation of samples

The GABA ELISA is a flexible test system for various biological sample types and samples. It is not possible to give a general advice how to prepare the samples. However, the following basics should help the researcher to fit the protocol to his specific needs:

⚠ For the determination of samples in a **range between 25 – 2500 ng/ml**, standards and controls should always be **diluted 1:3** with water [e.g. 100 µl standard + 200 µl water (deionized, distilled, or ultra-pure)]. This predilution of the standards has to be taken into account in the calculation of results.

The standards are diluted to make sure that the samples fall into the linear part of the standard curve. **Do not dilute samples!**

⚠ For the determination of samples in a **range between 75 – 7 500 ng/ml**, **do not dilute standards, controls or samples.**

- Avoid excess of acid: excess of acid might exceed the buffer capacity of the dilution buffer. A pH of 3.0 during the extraction is mandatory.
- It is advisable to perform a **Proof of Principle** to determine the recovery of GABA from the samples. Prepare a stock solution of GABA. Add small amounts (to change the native sample matrix as less as possible) of the stock solutions to the sample matrix and check the recovery.
- The sample volume determines the sensitivity of this test. Determine the sample volume needed to determine GABA in your sample by testing different amounts of sample volumes.

*If you need any support in establishing a protocol for your specific purposes, do not hesitate to contact the manufacturer directly!*

## 6.3 Test procedure (75 – 7 500 ng/ml)

### 6.3.1 Extraction

1.	Pipette <b>100 µl</b> of the <b>standards, controls</b> and <b>samples</b> into the appropriate wells of the <b>Extraction Plate</b> .
2.	Add <b>100 µl</b> of the <b>Diluent</b> to all wells. Cover plate with <b>Adhesive Foil</b> and incubate for <b>15 min</b> at <b>RT</b> (20 – 25 °C) on a <b>shaker</b> (approx. 600 rpm).
3.	<b>Discard</b> and blot dry by tapping the inverted plate on absorbent material. <b>Wash</b> each well with <b>500 µl</b> of <b>water</b> (deionized, distilled, or ultra-pure) and incubate for <b>5 min</b> at <b>RT</b> (20 – 25 °C) on a <b>shaker</b> (approx. 600 rpm).
4.	<b>Discard</b> the wash and blot dry by tapping the inverted plate on absorbent material.
5.	Pipette <b>400 µl</b> of <b>Elution Buffer</b> into the appropriate wells of the <b>Extraction Plate</b> . Cover plate with <b>Adhesive Foil</b> and incubate for <b>10 min</b> at <b>RT</b> (20 – 25 °C) on a <b>shaker</b> (approx. 600 rpm).
6.	Use <b>100 µl</b> for the subsequent <b>derivatization!</b>

### 6.3.2 Derivatization

1.	Pipette <b>100 µl</b> of the <b>extracted standards, controls</b> and <b>samples</b> into the appropriate wells of the <b>Microtiter Plate</b> .
2.	Pipette <b>10 µl</b> of the <b>NaOH</b> into all wells.
3.	Add <b>50 µl</b> of the <b>Equalizing Reagent</b> (fresh prepared before assay) to all wells and incubate for <b>1 min</b> on a <b>shaker</b> (approx. 600 rpm).
4.	Pipette <b>10 µl</b> of the <b>D-Reagent</b> into all wells.
5.	Cover plate with <b>Adhesive Foil</b> and incubate for <b>2 h</b> at <b>RT</b> (20 – 25 °C) on a <b>shaker</b> (approx. 600 rpm).
6.	Pipette <b>200 µl Q-Buffer</b> into all wells.
7.	Shake for <b>10 min</b> at <b>RT</b> (20 – 25 °C) on a <b>shaker</b> (approx. 600 rpm).
8.	<b>Use 50 µl for the subsequent ELISA!</b>

### 6.3.3 GABA ELISA

1.	Pipette <b>50 µl</b> of the <b>derivatized standards, controls</b> and <b>samples</b> into the appropriate wells of the <b>GABA Microtiter Strips</b> .
2.	Pipette <b>50 µl</b> of the <b>GABA Antiserum</b> into all wells and mix shortly.
3.	Cover plate with <b>Adhesive Foil</b> and incubate for <b>15 - 20 h</b> (overnight) at <b>2 - 8 °C</b> . <b>Alternatively incubate 2 h at RT (20 - 25 °C) on a shaker (approx. 600 rpm).</b>
4.	Remove the foil. Discard or aspirate the content of the wells. Wash the plate <b>3 x</b> by adding <b>300 µl</b> of <b>Wash Buffer</b> , <b>discarding</b> the content and <b>blotting dry each time</b> by tapping the inverted plate on absorbent material.
5.	Pipette <b>100 µl</b> of the <b>Enzyme Conjugate</b> into all wells.
6.	Incubate for <b>30 min</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm).
7.	Discard or aspirate the content of the wells. Wash the plate <b>3 x</b> by adding <b>300 µl</b> of <b>Wash Buffer</b> , <b>discarding</b> the content and <b>blotting dry each time</b> by tapping the inverted plate on absorbent material.
8.	Pipette <b>100 µl</b> of the <b>Substrate</b> into all wells and incubate for <b>20 - 30 min</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm). <b>Avoid exposure to direct sunlight!</b>
9.	Add <b>100 µl</b> of the <b>Stop Solution</b> to each well and shake the microtiter plate to ensure a homogeneous distribution of the solution.
10.	<b>Read</b> the absorbance of the solution in the wells within 10 minutes, using a microplate reader set to <b>450 nm</b> (if available a reference wavelength between 620 nm and 650 nm is recommended).

### 6.4 Test procedure (25 - 2 500 ng/ml)

#### 6.4.1 Extraction

1.	Pipette <b>300 µl</b> of the <b>diluted standards, controls</b> and <b>undiluted samples</b> into the appropriate wells of the <b>Extraction Plate</b> .
2.	Add <b>300 µl</b> of the <b>Diluent</b> to all wells. Cover plate with <b>Adhesive Foil</b> and incubate for <b>30 min</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm).
3.	<b>Washing step (2 cycles):</b> <b>Discard</b> and blot dry by tapping the inverted plate on absorbent material. <b>Add 1ml</b> of <b>I-Buffer</b> to each well and incubate the plate for <b>5 min</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm). <b>Discard</b> and blot dry by tapping the inverted plate on absorbent material. <b>Add 1ml</b> of <b>I-Buffer</b> to each well and incubate the plate for <b>5 min</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm).
4.	<b>Discard</b> and blot dry by tapping the inverted plate on absorbent material.
5.	Pipette <b>250 µl</b> of <b>Elution Buffer</b> into the appropriate wells of the <b>Extraction Plate</b> . Cover plate with <b>Adhesive Foil</b> and incubate for <b>10 min</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm).
6.	Use <b>100 µl</b> for the subsequent <b>derivatization!</b>

#### 6.4.2 Derivatization

1.	Pipette <b>100 µl</b> of the <b>extracted standards, controls</b> and <b>samples</b> into the appropriate wells of the <b>Macrotiter Plate</b> .
2.	Pipette <b>10 µl</b> of the <b>NaOH</b> into all wells.
3.	Add <b>50 µl</b> of the <b>Equalizing Reagent</b> (fresh prepared before assay) to all wells and incubate for <b>1 min</b> on a <b>shaker</b> (600 rpm).
4.	Pipette <b>10 µl</b> of the <b>D-Reagent</b> into all wells.
5.	Cover plate with <b>Adhesive Foil</b> and incubate for <b>2 h</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm).
6.	Pipette <b>150 µl</b> <b>Q-Buffer</b> into all wells.
7.	Incubate for <b>10 min</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm).
8.	<b>Use 25 µl for the subsequent ELISA!</b>

### 6.4.3 GABA ELISA

1.	Pipette <b>25 µl</b> of the <b>derivatized standards, controls</b> and <b>samples</b> into the appropriate wells of the <b>GABA Microtiter Strips</b> .
2.	Pipette <b>50 µl</b> of the <b>GABA Antiserum</b> into all wells and mix shortly.
3.	Cover plate with <b>Adhesive Foil</b> and incubate for <b>15 - 20 h</b> (overnight) at <b>2 - 8 °C</b> . <b>Alternatively incubate 2 h at RT (20 - 25 °C) on a shaker (approx. 600 rpm).</b>
4.	Remove the foil. Discard or aspirate the content of the wells. Wash the plate <b>3 x</b> by adding <b>300 µl</b> of <b>Wash Buffer, discarding</b> the content and <b>blotting dry each time</b> by tapping the inverted plate on absorbent material.
5.	Pipette <b>100 µl</b> of the <b>Enzyme Conjugate</b> into all wells.
6.	Cover plate with <b>Adhesive Foil</b> . Incubate for <b>30 min</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm).
7.	Remove the foil. Discard or aspirate the content of the wells. Wash the plate <b>3 x</b> by adding <b>300 µl</b> of <b>Wash Buffer, discarding</b> the content and <b>blotting dry each time</b> by tapping the inverted plate on absorbent material.
8.	Pipette <b>100 µl</b> of the <b>Substrate</b> into all wells and incubate for <b>20 - 30 min</b> at <b>RT (20 - 25 °C)</b> on a <b>shaker</b> (approx. 600 rpm). <b>Avoid exposure to direct sunlight!</b>
9.	Add <b>100 µl</b> of the <b>Stop Solution</b> to each well and shake the microtiter plate to ensure a homogeneous distribution of the solution.
10.	<b>Read</b> the absorbance of the solution in the wells within 10 minutes, using a microplate reader set to <b>450 nm</b> (if available a reference wavelength between 620 nm and 650 nm is recommended).

### 7. Calculation of results

Measuring range	GABA	
	Urine	
Plasma/Serum		25 - 2 500 ng/ml

The standard curve is obtained by plotting the absorbance readings (calculate the mean absorbance) of the standards (linear, y-axis) against the corresponding standard concentrations (logarithmic, x-axis). Use non-linear regression for curve fitting (e.g. spline, 4-parameter, akima).

⚠ *This assay is a competitive assay. This means: the OD-values are decreasing with increasing concentrations of the analyte. OD-values found below the standard curve correspond to high concentrations of the analyte in the sample and have to be reported as being positive.*

#### Serum/plasma

The read concentrations of **plasma samples** have to be **divided by 3**.

#### Urine samples and controls

The concentrations of the samples and controls can be read directly from the standard curve.

The total amount of GABA excreted in urine during 24 h is calculated as following:

$$\mu\text{g}/24\text{h} = \mu\text{g}/\text{l} \times \text{l}/24\text{h}$$

#### Conversion

$$\text{GABA (ng/ml)} \times 9.7 = \text{GABA (nmol/l)}$$

#### Expected reference value

It is strongly recommended that each laboratory should determine its own reference value.


Expected Reference Value	Spontaneous urine	230 - 1 290 µg/g creatinine
--------------------------	-------------------	-----------------------------


### 7.1 Quality control

The confidence limits of the kit controls are indicated on the QC-Report.



## 7.2 Typical standard curve

 Example, do not use for calculation!

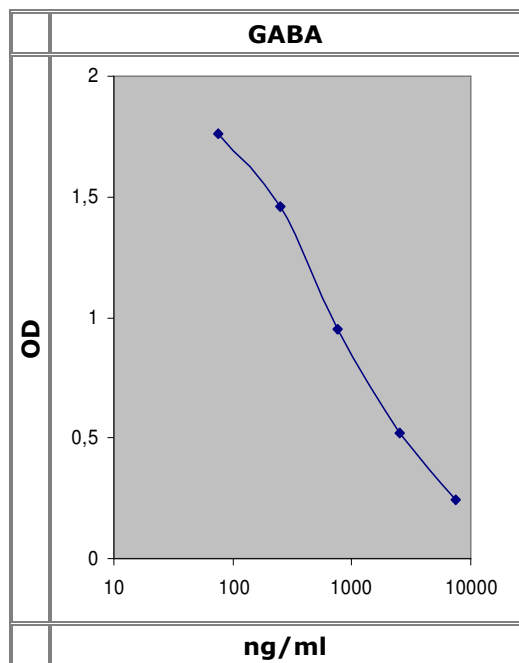

## 8. Assay characteristics

<b>Sensitivity</b> (lower limit of detection)	Urine (spontaneous)
	49 ng/ml

<b>Recovery</b>	Mean (%)	Range (%)	% Recovery after spiking
	104%	96 - 116%	

<b>Linearity</b>	Range (ng/ml)	Range (%)	Mean (%)
	35 - 4048	74-119	93

<b>Analytical Specificity (Cross Reactivity)</b>	<b>Substance</b>	<b>Cross Reactivity (%)</b>
		GABA
	β-Alanine	1.6
	α-Aminobutyric acid	< 0.09
	Glycine	< 0.09
	L-Glutamine	< 0.09
	β-Aminobutyric acid	< 0.09

<b>Precision</b>					
<b>Intra-Assay</b>			<b>Inter-Assay</b>		
Sample	Range (ng/ml)	CV (%)	Sample	Range (ng/ml)	CV (%)
1	318 ± 32	10	1	279 ± 35	12
2	723 ± 94	13	2	661 ± 73	11
3	2457 ± 110	4.9	3	1492 ± 117	7.8







## 9. References/Literature

- (1) Shmais et al. Mechanism of nitrogen metabolism-related parameters and enzyme activities in the pathophysiology of autism. *Journal of Neurodevelopmental Disorders* 4(1):4 (2012)
- (2) El-Ansary et al. Relationship between chronic lead toxicity and plasma neurotransmitters in autistic patients from Saudi Arabia. *Clinical Biochemistry*, 44(23):1116-1120 (2011)
- (3) Lee et al. Astrocytes Are GABAergic Cells That Modulate Microglial Activity. *Glia* 59:152-165 (2011)

Please use only the valid version of the Instructions for Use provided with the kit

- 
- ⚠ **For updated literature or any other information please contact your local supplier.**
  - ⚠ **The liability of the manufacturer shall be limited to the replacement of defective products. The manufacturer takes no liability for any damages or expenses arising directly or indirectly from the use of this product.**

### Symbols:

	Storage temperature		Manufacturer		Contains sufficient for <n> tests
	Expiry date	<b>LOT</b>	Batch code	<b>IVD</b>	For in-vitro diagnostic use only!
	Consult instructions for use	<b>CONT</b>	Content	<b>CE</b>	CE labelled
	Caution	<b>REF</b>	Catalogue number	<b>RUO</b>	For research use only!